

# ElectronRT DICOM Receiver for Patient Import

The decimal ElectronRT application supports importing DICOM patients via a DICOM listener/receiver. This guide details the process for enabling and configuring this method of DICOM patient import into the eRT application.

## DICOM Receiver

The following guide details how to download, install, and configure the ElectronRT DICOM Receiver to automatically accept and import files into the ElectronRT application for import.

### Download and Installation



1. Download the ElectronRT DICOM Receiver via:
2. Extract the ElectronRT\_dicom\_receiver.zip file to an appropriate directory of your choosing (e.g.: C:\ElectronRT\_DICOM\_Receiver)
3. Edit the receiver\_config.json file to set the following fields:
  1. **local\_ae\_title**: The name of the listener (Note: this is not explicitly enforced, it's only for reference)
  2. **local\_port**: The local port for the listener to monitor on
  3. **timeout**: The timeout, in seconds, for which to wait for files/connections. The default value is an appropriate setting.
  4. **storage\_location**: The shared network location to save files to that the ElectronRT app will be able to access and monitor (refer to [Importing a Patient from a DICOM Receiver](#) for more details on this process within the eRT application).

### Running Modes

The ElectronRT DICOM Receiver has two options for running:

#### 1. Running as a Windows Service (recommended)

The following scripts can be used to add, remove, or restart the Windows Service for the ElectronRT DICOM Receiver.

**Note:**

Administrator permissions are required to modify Windows Services, so each of the provided service management scripts



below must be run as an administrator.

- **service\_install.bat**
  - Installs the ElectronRT DICOM Receiver as a Windows Service
- **service\_uninstall.bat**
  - Removes the ElectronRT DICOM Receiver from the Windows Services
- **service\_restart.bat**
  - Restarts the Service if changes are made to the configuration file.

## 2. Running as a Stand Alone Application

The ElectronRT DICOM Receiver can be run as a stand alone application. This option does not require administrative privileges.

1. Open Windows Explorer to the ElectronRT DICOM Receiver installation directory
2. Run the ElectronRT DICOM Receiver .exe to start the receiver as configured

Notes:

- Any time the Computer is restarted (e.g.: windows updates) the stand along application will need to be manually run.
- Any time the receiver\_configuration.json file is changed, the application will need to be manually restarted to load the new configuration

---

## ElectronRT DICOM Monitoring and Patient Import


The following items detail the steps required to configure and use the patients received from the ElectronRT DICOM Receiver within the ElectronRT application:

1. Users must set the DICOM Import Monitoring Directory within the [Site Configuration's DICOM Settings](#) block that corresponds to the storage\_location field set for the ElectronRT DICOM Receiver.
2. Once the monitoring directory has been set the [Importing a Patient from a DICOM Receiver](#) section provides details how to import patients received from the ElectronRT DICOM Receiver.



**Note:**

Patient files stored temporarily within the DICOM Import Monitoring Directory are unencrypted DICOM files that may contain PHI. Please ensure this folder is located on your facility's secured network and accessible only by approved staff.

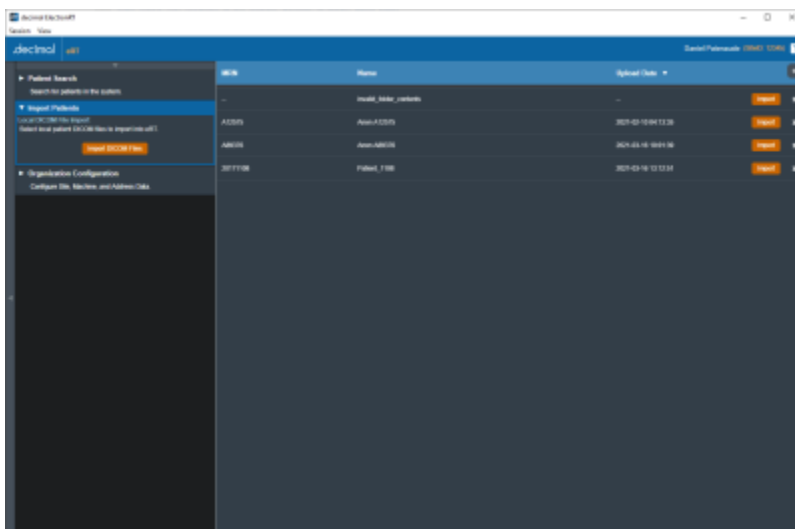

The screenshot shows the ElectronRT DICOM Receiver interface. On the left, there is a sidebar with navigation options: 'Patient Search', 'Import Patients', and 'Organization Configuration'. The 'Import Patients' section is active, showing a list of patients. The main area displays a table with columns for 'ID', 'Name', and 'Updated Date'. There are three rows of patient data, each with an 'Import' button and a close icon.

ID	Name	Updated Date
---	import_test_patient	---
A12345	Alan A12345	2021-03-10 04:12:38
A6789	Ann A6789	2021-03-10 04:12:38
2017128	Patrick F188	2021-03-10 12:12:38

Fig. 1: DICOM Receiver Patients

From:

<https://apps.dotdecimal.com/> - **decimal App Documentation**

Permanent link:

[https://apps.dotdecimal.com/doku.php?id=electronrt:userguide:dicom\\_receiver&rev=1617056021](https://apps.dotdecimal.com/doku.php?id=electronrt:userguide:dicom_receiver&rev=1617056021)

Last update: **2021/07/29 18:22**