


Importing Patient Data

Now that a patient has been uploaded from DICOM to thinknode ISS and an RKS entry created, the Planning App should recognize that a new patient is available to import into a Planning patient.

1. Open the Astroid Launcher and login (If you have already logged into Astroid start at step 6)
2. Select your realm
3. A list of available apps will be listed on the right, select *Planning* from this
4. If you see an Install button click it and wait for the version to install. You will know it is installed when you see a LAUNCH button
5. Click the LAUNCH button. The version of planning that is installed in your realm will now open
6. Click on the Imports

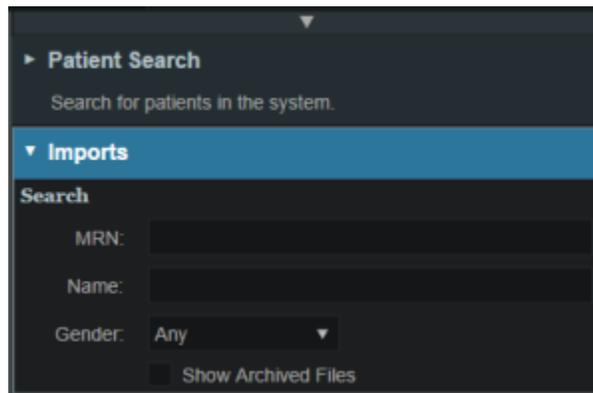


7. Select the CT image set from the list of available files for import


Modality	MRN	Name	Upload By	Upload Date
Structure Set	111114	SBRT PROSTATE	Keitt Mobile	2017-01-05 12:14:47
CT Image Set	111114	SBRT PROSTATE	Keitt Mobile	2017-01-05 12:14:54

8. Ensure that the MR is correct

1. If MR needs to be changed you may edit it by choosing the *Edit* button to the left

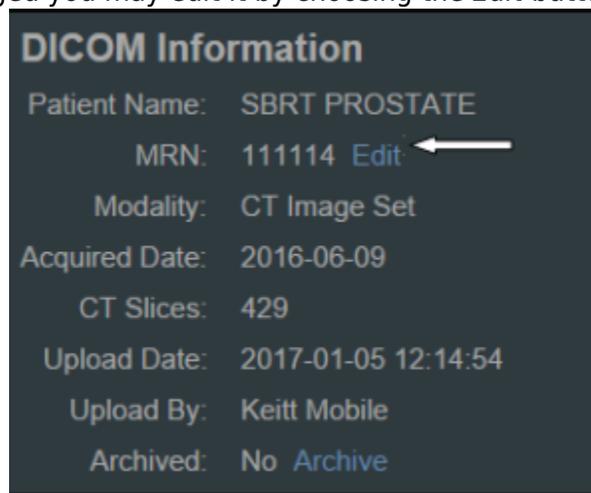

9. Click the *Create Patient* button to start the import process

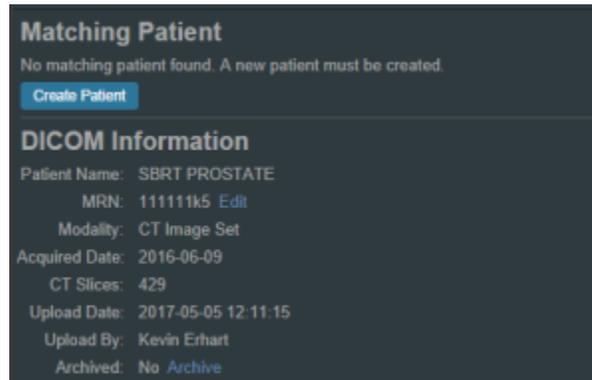

Matching Patient

No matching patient found. A new patient must be created.

[Create Patient](#)

DICOM Information

Patient Name: SBRT PROSTATE
MRN: 111111k5 [Edit](#)
Modality: CT Image Set
Acquired Date: 2016-06-09
CT Slices: 429
Upload Date: 2017-05-05 12:11:15
Upload By: Kevin Erhart
Archived: No [Archive](#)

10. In the control pane on the left hand side, the image snapshot will be automatically selected based on the structure set DICOM UID information.
11. Fill in the Patient Intent information and select the appropriate HU to RSP curve (as shown below)

Intent Data

Type *: Curative

Label: intent_curative_2017Jan4

Treatment Site *: Prostate_Protocol

Narrative:

Protocol: 123456 New Protocol

Body System *: Male Reproductive System

Body Part *: Prostate

ICD-10 Code: DV004ZZ

RSP Data

HU to RSP Curve*: Scanner1; 120 kVp; FOV [0, 1000]

Import Structure Set

Structure Set: Date: 2016-06-09

Import Structures

Treatment Site: Prostate_Protocol

Patient Structure: Skin

Variant Label: variant_1_2017Jan4

<input checked="" type="checkbox"/> Bladder neck (custom)	Importing new structure
<input checked="" type="checkbox"/> Testes (custom)	Importing new structure
<input checked="" type="checkbox"/> 2cm (custom)	Importing new structure
<input checked="" type="checkbox"/> Skin (matched)	Importing new structure
<input checked="" type="checkbox"/> penile bulb (custom)	Importing new structure
<input checked="" type="checkbox"/> Neurovascular Bu (custom)	Importing new structure
<input checked="" type="checkbox"/> Prostate (matched)	Importing new structure
<input checked="" type="checkbox"/> PTV (custom)	Importing new structure
<input checked="" type="checkbox"/> Seminal Vesicles (custom)	Importing new structure
<input checked="" type="checkbox"/> Bladder (matched)	Importing new structure
<input checked="" type="checkbox"/> Rectum (matched)	Importing new structure
<input checked="" type="checkbox"/> Urethra (custom)	Importing new structure
<input checked="" type="checkbox"/> Bowel (custom)	Importing new structure
<input checked="" type="checkbox"/> Left Femoral Hea (custom)	Importing new structure
<input checked="" type="checkbox"/> Right Femoral He (custom)	Importing new structure

Archive DICOM on import

Create Patient Cancel

12. You will see a list of the imported structures. Here you may choose whether or not to import each structure by checking or unchecking the box beside each structure name.

13. You also have the ability to assign or edit any structures that are shown as *custom*, which indicates the name did not exactly match a directive structure from the treatment site template list you specified during patient creation.
 1. Matched, Assigned, and Custom structures are designated with corresponding tags at the end of the structure name in the structure list.
 2. Assigning a custom structure to a defined directive structure will result in the imported structure inheriting all the predefined structure properties (e.g. name, type, color)
 3. For all custom structures the type is by default set to "Other" unless it contains the letters "TV" (as in PTV or CTV), in which case it is assigned the type of "Target"; this may be changed here if needed
14. Click the "Create Patient" button to create the patient and import the CT Images and Structures into it.
15. The patient is now created and all available data has been imported, so it is time to proceed with entering the prescription information
16. Click on the *Back to Import* button

From:

<http://apps.dotdecimal.com/> - **decimal App Documentation**

Permanent link:

<http://apps.dotdecimal.com/doku.php?id=planning:userguide:tutorials:importing&rev=1484084958>

Last update: **2021/07/29 18:24**

