


# Optimization Objectives

*Objectives* communicate to the optimizer the goals that are important to strive for in your plan. *Objectives* are set at the *Plan* level under *Plan Constraints/Objectives* and they apply to the total, combined dose from all beams. *Objectives* are not given any relative importance at this point (i.e. their order within the list is not meaningful). The *Objectives* drive the solution of the Multi Criteria Optimization (MCO) and for each *Objective*, a corresponding *Navigation Slider* will be presented to allow for exploration of trade-offs in the case of competing objectives (for more information about the MCO process and how objective importance/weighting is handled in Astroid refer to [this article](#)).

The following objective selections are available in Astroid:

- **min\_max**: Minimize the maximum dose within a structure (drive dose down)
- **max\_min**: Maximize the minimum dose within a structure (drive dose up)

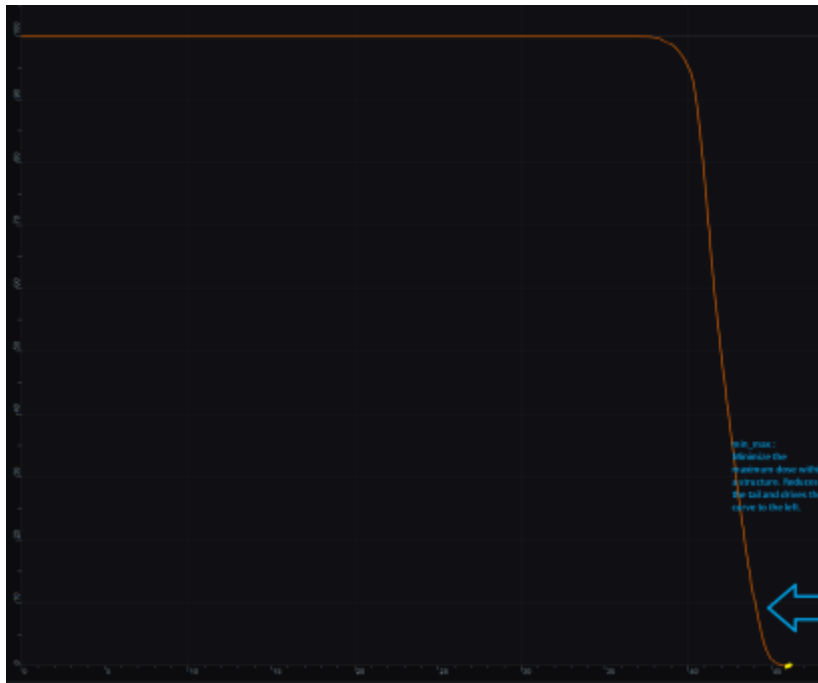


min\_max: Minimize the Max Dose




max\_min: Maximize the Min Dose

- **min\_mean:** Minimize the mean dose within a structure (drive dose down)
- **max\_mean:** Maximize the mean dose across the structure (drive dose up)
- **min\_overdose:** Minimize the high dose within a structure
  - Dose will be driven down only until the specified limit is reached (this is often more relevant that min\_max, since it may not be beneficial to continue minimizing beyond a certain dose level)
- **min\_underdose:** Minimize the low dose within a structure
  - Dose will be driven up only until the specified limit is reached (this is often more relevant that max\_min, since it may not be beneficial to continue maximizing beyond a certain dose level)

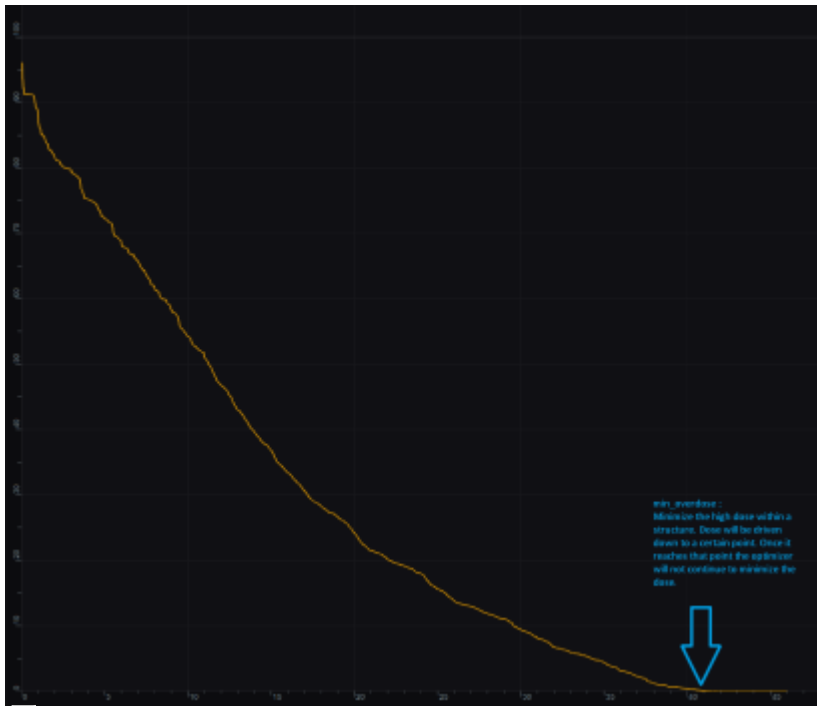

min\_overdose: Minimize the high dose

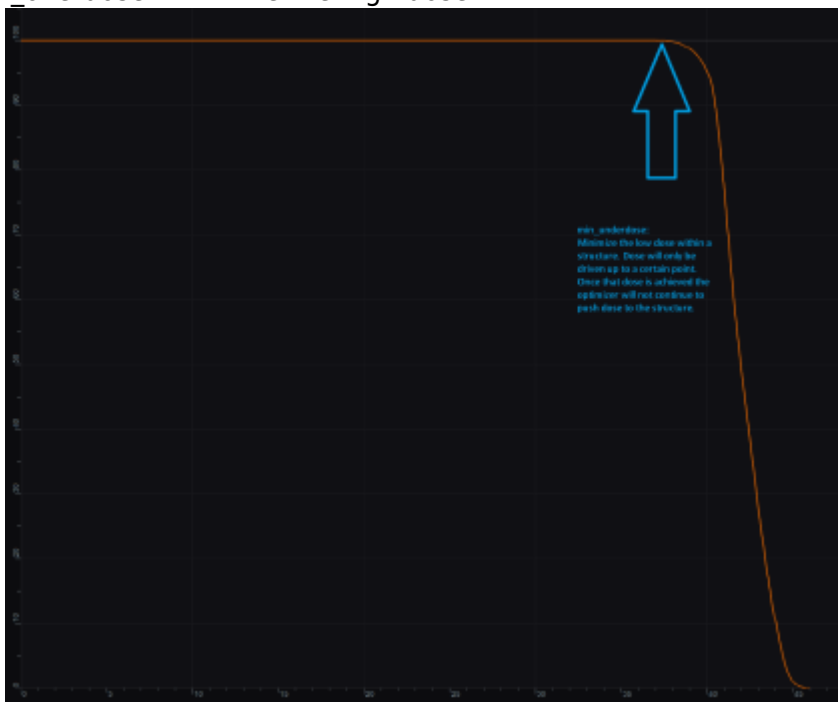

min\_underdose: Minimize the low dose

## Working with Objectives

1. Open the *Objectives* sub-block contained in the *Plan Constraints/Objectives* block
2. Choose a structure to which you wish to apply objectives
3. Check the boxes to activate the desired objectives for the structure and then set the dose level if applicable

Objectives

☒ Rectum ✕

☒ min\_max  
35 Gy(RBE)

☐ min\_mean

☒ min\_overdose

☒ PTV ✕

☐ min\_max

☐ max\_min

☐ min\_mean

☐ max\_mean

☒ min\_underdose  
45 Gy(RBE)

☒ min\_underdose  
Gy(RBE)

Add Structure ▼

OK Cancel

Once all the *Objectives* have been set, the user is ready to run the MCO solver, which is performed in the *Navigation* block.

From:  
<http://apps.dotdecimal.com/> - decimal App Documentation

Permanent link:  
[http://apps.dotdecimal.com/doku.php?id=planning:userguide:tutorials:optimization\\_objectives&rev=1487365465](http://apps.dotdecimal.com/doku.php?id=planning:userguide:tutorials:optimization_objectives&rev=1487365465)

Last update: 2021/07/29 18:25

