
Prostate Plan Walkthrough

Patient Creation

- 1. Open the Astroid Launcher and login
- 2. Select your realm
- 3. A list of available apps will be listed on the right, select Planning from this
- 4. If you see an Install button click it and wait for the version to install. You will know it is installed when you see a LAUNCH button
- 5. Click the LAUNCH button. The version of planning that is installed in your realm will now open
- 6. Click on the Imports
- 7. Select the CT image set (SBRT Prostate) from the list of available files for import
- 8. Ensure that the MR is correct
 - 1. If MR needs to be changed you may edit it by choosing the Edit button to the left
- 9. Click the Create Patient button to start the import process



- 10. In the control pane on the left hand side, the image snapshot will be automatically selected based on the structure set DICOM UID information.
- 11. Fill in the Patient Course information and select the appropriate HU to RSP curve (as shown below)

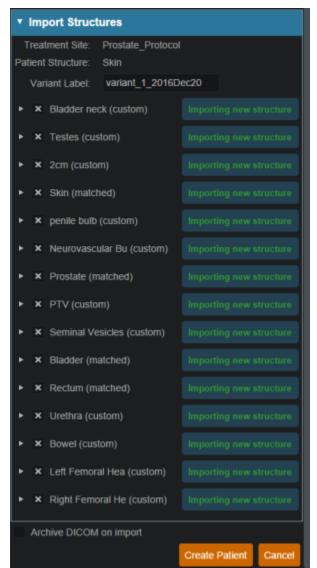

- 12. You will see a list of the imported structures. Here you may choose whether or not to import each structure by checking or unchecking the box beside each structure name.
 - 1. For this case, we will import all available structures and there is nothing to change on this page
- 13. You also have the ability to assign or edit any structures that are shown as *custom*, which indicates the name did not exactly match a directive structure from the treatment site template list you specified during patient creation.
 - 1. Matched, Assigned, and Custom structures are designated with corresponding tags at the end of the structure name in the structure list.
 - 2. Assigning a custom structure to a defined directive structure will result in the imported structure inheriting all the predefined structure properties (e.g. name, type, color)
 - 3. For all custom structures the type is by default set to "Other" unless it contains the letters "TV" (as in PTV or CTV), in which case it is assigned the type of "Target"; this may be changed here if needed
- 14. Click the "Create Patient" button to create the patient and import the CT Images and Structures into it.
- 15. The patient is now created and all available data has been imported, so it is time to proceed with entering the prescription information
- 16. Click on the *Back to Import* button


Prescription

- 1. Click the Patient Search task
- 2. Click the entry from the table of patients that corresponds to your newly imported patient
- 3. Prescription information is stored in the Course
- 4. Click edit under the Course entry in the patient overview tree
- 5. Fill in Clinical Goals
 - 1. Choose the structure from the dropdown to add your goal
 - 2. In this example we will set a minimum dose to the PTV at 79.2Gy and the maximum dose at 85.5Gy as shown below
- 6. Next proceed to *Prescriptions*
 - 1. Select New Prescription
 - 2. For this example the dose will be 79.2Gy in 44 fractions to the PTV
 - 3. *Label* and *Description* are free text fields that allow you to "name" each Prescription and provide any description or notes necessary to distinguish between each in the case of multiple prescriptions. You must enter a "name" in the *Label* in order to proceed. You are free to enter your own values in these fields for this walkthrough


Ŧ	Course: course	_2017-May-08				edit
	Name:	course_2017-	May-08			
	Description:					
	Physician:		•			
	Treatment Site:	Prostate_Prote				
	Clinical Goa	ls				
	PTV					×
	min:	79.2	Gy(RBE)	×		~
	max	85.5	Gy(RBE)			
	min mean;	Add Statement				
	max mean:					
	min DVH:					
	max DVH:					
	Add Structu	re 🔻				
	Prescription	5				
	Initial					•
	Labe	i: prostate				
	Description					
	Cressinghild					
	Colo	c 🔳 💿 💿			• •	
	Fractions	ε 44				
	Prescription	n: 79.2 Gy	(RBE) to	PTV	• ×	
		Add	٠			
					Done Ca	ncel
	New Prescri	ption				
					Done	Cancel

- 7. Click Done to complete the Course editing
- 8. You can now click on the patient's name, "SBRT PROSTATE", on the top line to return to the Patient Overview tree

- 1. The required *Course* and *Patient Model* information was selected during import, so now we can move to creation of a treatment *Plan*
- 2. From the Patient Overview tree, click the Add Plan button under the Patient Model entry
 - 1. Name the plan and click OK

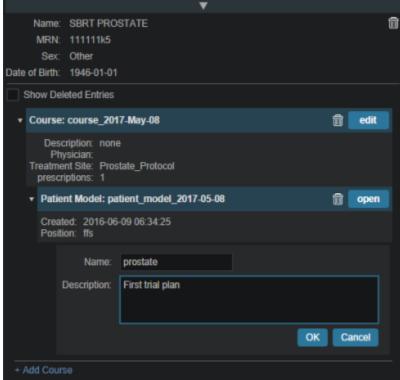

- 2. This creates an empty plan with its prescription set to fulfill all portions of the Course Prescription
- 3. Now open the new plan by clicking the *Open* button under the new plan entry in the Patient Overview tree



General Plan Parameters

- 1. We will start our plan by reviewing the General / History block information
- 2. Click the General / History heading to expand this block
 - 1. Notice here that our empty plan starts out with its prescription set to fulfill all portions of the Course Clinical Goals and Prescriptions
 - 2. If a plan will only fulfill a portion of the Prescription, then this information should be edited to reflect this, otherwise just proceed past this block
- 3. In this case, we will be fulfilling the entire prescription with a single plan, so no editing is needed
- 4. Generating our plan will now progress to the *Patient Geometry* block, where we will create any points or planning structures that are needed (if not created in contouring software), such as a


combination of the left and right femoral heads (see Structure Geometry for details on how to create structures)

- 5. We will create a point to use for the isocenter (note this step is done for illustration purposes and is not necessary for most plans)
 - 1. Select a type of isocenter and create the point at the centroid of the PTV

Points					
	Create New Point				
Create Point					
 General 					
	Isocenter 🔹				
Description:					
▼ Geometry					
 Explicit Create a point at a specified location. Centroid Create a point at the centroid of a structure. 					
Structure PTV Position: (-3.3)					
	jump to point po				

- 2. Click DONE at the bottom of the page
- 6. Next we will move on to defining the HU to Proton Relative Stopping Power (RSP) conversion
- 7. Click to open the RSP Image block
- 8. If any density overrides are needed they are entered here in the RSP Image block
- 9. If the HU to RSP curve was not chosen upon patient import the user may do so at this point
- 10. We do have any density overrides to apply for this case and the proper HU curve has already been selected, so we can move past this block for this example, so click *Cancel* to close this block
- 11. We are now ready to define the dose calculation grid (see Defining the Dose Grid for a detailed explanation)
- 12. Click to open the Calculation Grid block
- 13. Create a grid by performing the following steps:
 - 1. Set the base grid resolution to 8 mm
 - 2. Click Add Structure and select the "2cm" structure
 - 1. Set the size to 4 mm
 - 3. Add the PTV in the same manner and the sizes to 2 mm

6/14

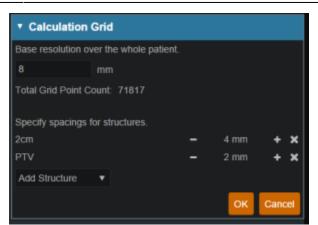

- 4. The Prostate is included in the PTV volume so there is no need to set a separate grid size
- 5. Click OK

Beams

- 1. We are now ready to begin defining the treatment beams
- 2. Click to expand the *Beams* block (see Creating a New Beam for detailed explanation)
 - 1. Before defining individual beams, we will first set some shared beam properties
 - 2. Set the Treatment Room by choosing "Gantry 2" from the dropdown

OK Cancel

- 3. Click OK
- 4. Expand the *Spot Placement* sub-block and set the following values (note these are the plan level spot placement parameters, so it will apply to all our beams, unless we specifically override the values within an individual beam)
 - 1. Lateral margin- 15 mm
 - 2. Distal margin- 10 mm
 - 3. Spot spacing- 1 sigma
 - 4. Layer spacing- 0.8 Distal W80

▼ Beams				
Treatment Room				Gantry 2
Spot Placement Parameters:				
Lateral Margin:	15	mm		
Distal Margin:	10	mm		
Spot Spacing:	1	Sigma	•	
Layer Spacing:	0.8	Distal W80	•	
			ОК	Cancel

- 5. Click OK
- 6. Now we are ready to make our beams

7. Start by clicking Create New Beam

▼ Beams	
Treatment Room	Gantry 2
Spot Placement Parameters	using user values
PBS Beams	
Create New PBS Beam	

- 1. Enter the following for each beam
 - 1. General
 - 1. Select the PTV as the target and if desired, enter a description for the beam, for other selections leave the defaults (see Structure Geometry)

▼ General	
Color:	
Label:	
	× automatically generate label
Target:	PTV V
Description:	

- 2. Approach
 - 1. At this point the user will specify the geometry of the beam by setting the isocenter as well as the gantry and couch angles
 - Two beams at gantry angles of 90 and 270, respectively, will be used here, which is typical (+/- 5 degrees) for standard prostate plans such as this example
 - 3. Couch angle of 0 is used here for each beam
 - 1. You may use the sliders, the +/- buttons, or simply type in the values to adjust these angles

• Approach	1			
Isocenter:	p1 - Centroid o Prostate	f 🔻		
Gantry Angle:	90	deg		
Couch Angle:	0	deg	- •	
			- +	

- 3. Snout
 - 1. Depending on the size of the prostate a 10-12cm snout should be adequate, in this example select the 12cm Snout option
 - 2. If the pelvic nodes need to be included, the user may need to increase the snout size to the 18 or 25cm snout


 Snout 	
Snout	12 cm
	18 cm
	25 cm
	30x40 cm

- 4. Aperture (if desired)
 - 1. If there is the need to use an Aperture for sharper penumbra the user can do so at this time (see Creating an Aperture)
 - 2. Note that Astroid has the ability to utilize an Aperture with pencil beam scanning for both SFUD and IMPT plans
 - 3. For this plan, no apertures are necessary
- 5. Shifter
 - 1. Simply choose a shifter from the list if one is needed
 - 2. For this plan, no shifters are necessary

 Shifter 		
Shifter:	none	
	30 mm	
	47 mm	
	80 mm	

6. Air gap

- 1. The air gap is specified as the distance from the final beamline device (aperture or shifter) or the snout end if no devices are present
- 2. The view automatically shifts to the 3D view when entering this sub-block and you can adjust the air gap to ensure patient collisions are avoided
- 3. The default air gap of 30 mm is sufficient for both beams in this example
- 7. Spot placement
 - 1. Since we want both beams to use the same spot settings, we have those at the plan level and there is no need to edit the spot placements here for the beams
- 8. DRR options
 - 1. The Proton DRRs shown in the *Beam* task are generally used to help determine appropriate treatment angles
 - 2. In cases such as these, appropriate angles are readily determined and there is no need to utilize the DRR sub-task
 - If you wish to explore this feature however, you may choose one of the preset *Density Presets* from the drop down or manually set the *level, window, min HU* and *max HU* or go into *Advanced Options* for additional control of the DRR's
 - 2. These proton DRRs are used only for visualization purposes and will have no effect on the plan construction process

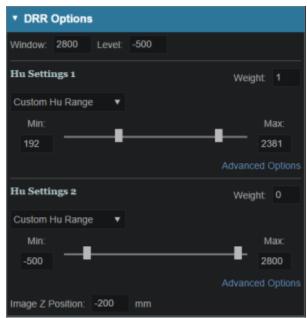

- 2. Click Done to complete the first beam
- 3. After creating the first beam (at gantry angle 90) it is recommended that you *Clone* it and simply change new beam's ganry angle to save time in creating the second beam (the *Clone* button is available under a beam when it is selected for viewing from the list of beams)

▼ Beams	
Treatment Room	Gantry 2
Spot Placement Parameters	using user values
PBS Beams	
b1 - G270 C0; 12 cm; no	shifter; 🧧
Beam Information Description:	
Isocenter:	p1 - Centroid of PTV
Gantry Angle:	270 deg
Couch Angle:	0 deg
Target:	PTV
Air Gap:	30 mm
Entrance Z:	210 mm
Snout	12 cm
Aperture:	none
Shifter:	none
PBS Spot Placement	
using plan settings:	
	Clone Edit Delete
Create	e New PBS Beam

4. Once you have *Cloned* the beam choose the *Edit* button to make changes to the gantry angle

10/14

PBS Beams					
b1 - G270 C0; 12 cm; no	b1 - G270 C0; 12 cm; no shifter;				
b2 - G270 C0; 12 cm; no	b2 - G270 C0; 12 cm; no shifter;				
Beam Information Description: Isocenter	p1 - Centroid of PTV				
Gantry Angle:					
Couch Angle:	-				
Target:	PTV				
Air Gap:	30 mm				
Entrance Z:	210 mm				
Snout:	12 cm				
Aperture:	none				
Shifter:	none				
PBS Spot Placement					
using plan settings:					
	Clone Edit Delete				
Creat	Create New PBS Beam				


1. Note for more complex plans, there are often additional parameters to change (such as the aperture and the air gap) when creating additional beams via the *Clone* option

Optimization

- 1. With the two beams completely defined, we can now move on organizing our treatment fraction groups and specifying the constraints and objectives for the treatment
- 2. Open the *Optimization* block (see Astroid Optimization for a detailed explanation of *Optimization*, *Feasibility* and *Constraints*, as well as *Running the Optimizer*)

Fraction Group

1. Choose *Create a New Fraction Group* under the *Fraction Group* block (See Fraction Groups for a more detailed explanation)

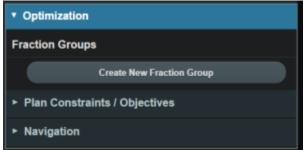

- 1. Enter a Fraction Count of 44
- 2. Add a new Target to the *Target List* by clicking *Add Target*
 - 1. Set the Target to the PTV
 - 2. Add the following Beam Set

- 1. In this case we will use an IMPT approach so add both the G90 and G270 beams in this same beam set
- 3. Constraints associated with this target
 - 1. Click the Add Structure drop down and choose the PTV
 - 2. Add a min dose constraint of 79.2 Gy (1.8 Gy per fx)
 - 3. Add a max dose constraint of 85.5 Gy
- 4. At this point your *Fraction Group* should appear as shown below

e Fraction Group				
Color:		• • • •	•••	
escription:				
on Count:	44			
Phase:	initial	Ŧ		
Group Constraints:		e 🔻		
List				
	Add Anot	her Target		
Target:	PTV	•		
am Sets:	▼ beam set			
	b2 - G90 (CO; 12 cm; n n		×
nstraints.	Max: Min Mean: Max Mean:	85.5 add statem add statem	ent	x
	Color: escription: on Count: Phase: onstraints: List	Color: Color: 44 Phase: initial on Count: 44 Phase: initial onstraints: Add Structur List Add Anot Target: PTV am Sets: • beam set b1 - G270 b2 - G90 (add beam set • PTV Min: Max: Min Mean: Max Mean:	Color: escription: 44 Phase: initial Phase: Add Structure List Add Structure Add Another Target Target: PTV Add Another Target beam set b1 - G270 C0; 12 cm; n add beam add beam add beam add beam Add Structure PTV Min: 79.2 Max: 85.5 Min Mean: add statem Max Mean: add statem	Color: escription: 44 Phase: initial Phase: Add Structure List Add Structure Add Another Target Target: PTV Add Another Target b1 - G270 C0; 12 cm; no shifter; b2 - G90 C0; 12 cm; no shifter; b2 - G90 C0; 12 cm; no shifter; add beam set PTV Min: 79.2 cyteer) X Max: 85.5 cyteer) X Max: 85.5 cyteer) X

3. Click *Done* to complete the Target entry and then *Done* again to complete the *Fraction Group*

Constraints and Objectives

- 1. This is our only Fraction Group for this plan, so we'll move on to the plan level constraints and objectives
- 2. Open the Plan Constraints/Objectives block
 - 1. First we'll enter the *Constraints* for the planning (target) volumes and a global maximum constraint
 - 1. Remember these are the "hard stops/non negotiables" for the plan
 - 2. These doses will be decided per the users' department protocols

- 3. For this case do the following:
 - 1. Click Add Structure and select Skin
 - 1. Add a max set to 85.5
 - 2. Click OK
 - 3. Note that we already have PTV dose constraints at the Fraction Group Target level, so no additional one are needed here



After the target constraints have been entered, it's generally good practice to test the plan feasibility. The Feasibility calculation is run by clicking *calculate* in the Feasibility block at the bottom of the *Plan Constraints/Objectives* sub-block. The Feasibility calculation is based solely on the constraints and it should be used to ensure there is a possible solution (plan) that can meet the specified constraints. The Feasibility calculation may be an iterative processes in order to get appropriate constraint, check the feasibility, then progressively tighten the constraint and check the feasibility until the plan is no longer feasible. It is recommended practice to start by obtaining a feasible plan utilizing only target constraints then add OAR constraints as desired. Remember, using a narrow range of constraints can improve the optimizer performance and improve the resolution of the Pareto surface navigation.

1. Run the Feasibility by clicking the calculate link

Feasibility		
not calculated		
calculate		

- 1. The feasibility should return as passing, if not, please confirm your plan parameters match those shown throughout this walkthrough and try again
- 2. Now with the target constraints set, we'll move on to our OAR's
 - 1. Again these will be set per department protocol
 - 2. For this example create the following OAR constraints:
 - 1. Rectum max mean 50 Gy
 - 2. Bladder max mean 60 Gy

 Plan Constraints / Objectives 				
Constraints structure	type	dose _{Gy(RDE)}		
SkinRectumBladder	max max_mean max_mean	85.5 50 50 Edit		

- 3. Run Feasibility again
 - 1. The feasibility should return as passing again, if not, please confirm your plan parameters match those shown throughout this walkthrough and try again
- 4. With narrow constraints set and feasibility established, we will now turn our attention to Objectives

- 1. *Objectives* are the goals that you would like to achieve and these will be the driving forces for the optimizer
- 2. Click Edit under the Objectives section
- 3. For this example we will use the following objectives:
 - 1. Rectum min_mean (Minimize the mean dose to the Rectum)
 - 2. Testes min_max (Minimize the maximum dose to the Testes)
 - 3. Left & Right Femur min_overdose 45 Gy (Minimize the amount of the structure the receives dose above 45 Gy)
 - 4. PTV min_max (Minimize the maximum dose within the PTV)
 - 5. PTV max_min (Maximize the minimum dose within the PTV)

Objectives	
Rectum min_max min_mean min_overdose	ĸ
Testes > × min_max max_min min_mean max_mean min_overdose min_underdose	ĸ
Left Femoral Hea min_max max_min min_mean max_mean min_overdose min_underdose 45 Gyree	×
Right Femoral He Right Femoral He min_max min_mean min_mean min_overdose min_overdose min_underdose	×
PTV X min_max Min_mean min_mean min_overdose Min_underdose	×
Add Structure	

- 5. Click OK to complete the Objectives
- 6. We are now ready to run the MCO, by opening the *Navigation* sub-block and clicking the *calculate* link
 - 1. This may take up to 20 minutes for this plan depending upon your available cloud services resources
 - 2. Keep in mind that even though this process may take some time the planner will be able to make adjustments easily in the Navigation without running a new plan

Navigation

- 1. Once the MCO has been completed, you can adjust the relative importance of the objectives using the slider bars in the *Navigation* block (see Astroid Optimization *Navigating the Solutions* for a detailed explanation of using the slider bars)
 - 1. Adjust the slider bars in the *Navigation* block to find what you feel is the optimal plan for this case
 - 1. Note: All of these adjustments are made without having to run a new plan
 - 2. If you find a plan that you like, but wish to continue exploring further, you can click the *Save* button to save the current slider state and then continue exploring
 - 3. You may return to the last saved state at any time by clicking the Reset button
 - 4. The Cancel button will close the navigation block, reverting back to the last Saved state

۲	▼ Navigation						
٠	Current Plan						
	Rectum 19.02	min_mean	28.08 < 34.87				
	Testes 0.00	min_max	0.00 < 0.01				
	Left Femoral Hea	min_overdose					
	Right Femoral He 0.00	min_overdose	-				
	PTV 80.18	min_max	83.54 < 85.50				
	 PTV 79.20 	max_min					
	Reset Save Dose	•	Save Cancel				

- 2. The plan is ready for physician review at this point
 - 1. Physicians often find it useful to Navigate the solution and explore trade-offs in real time, which can often alter the traditional physician approval process into an interactive, real-time trade-off analysis and on the spot plan approval
- 3. After the physician has decided on a treatment plan the user may then proceed to export the chosen plan to the EMR
 - 1. Note that these standard (non-plan specific) features are covered in other guides and not repeated herein

From: https://apps.dotdecimal.com/ - decimal App Documentation

Permanent link: https://apps.dotdecimal.com/doku.php?id=planning:userguide:walkthroughs:prostate_plan&rev=1494345262

Last update: 2021/07/29 18:25